

" 30 Min. Battery Backup "
First time in the world !

MISPA*///*-i

Intelligent Nephelometry Technology
Smart Card with Automated Calibration
Economic 26 Parameter Assay



AGAPPE

MISPAW*-i*

SERUM PROTEIN ANALYZER

The MOST INTELLIGENT SERUM PROTEIN ANALYZER

Parameters

ASO	30T
CRP	30T
RF	30T
HbA1c	30T
IgE	30T
Microalbumin	30T
Lp(a)	30T
Cystatin C	30T
Ferittin	30T
Apo A	30T
Apo B	30T
Ceruloplasmin	30T
IgA	30T
IgG	30T
IgM	30T
C3	30T
C4	30T
Transferrin	30T
Kappa Light Chain	30T
Lambda light chain	30T
Pre albumin	30T
Alpha 1 acid glycoprotein	30T
Alpha 2 Macro globulin	30T
Alpha 1 Antitrypsin	30T
Hapto globin	30T
D-Dimer	30T

Specifications


Measurement Method	: Nephelometry
Light Source	: Laser
Operating Temperature	: 15-30°C
Printer	: Built in, Thermal
Power supply	: 220 V, 60 W, 47-50 Hz
Calibration	: IC Card

Free Accessories along with Mispa - i

Pipette with Sensor	- 1
Micro Pipettes	- 2

Free Accessories along with Reagent Kit

Smart Card	- 1
Reaction Cuvettes	- 30
Micro Tips	- 90

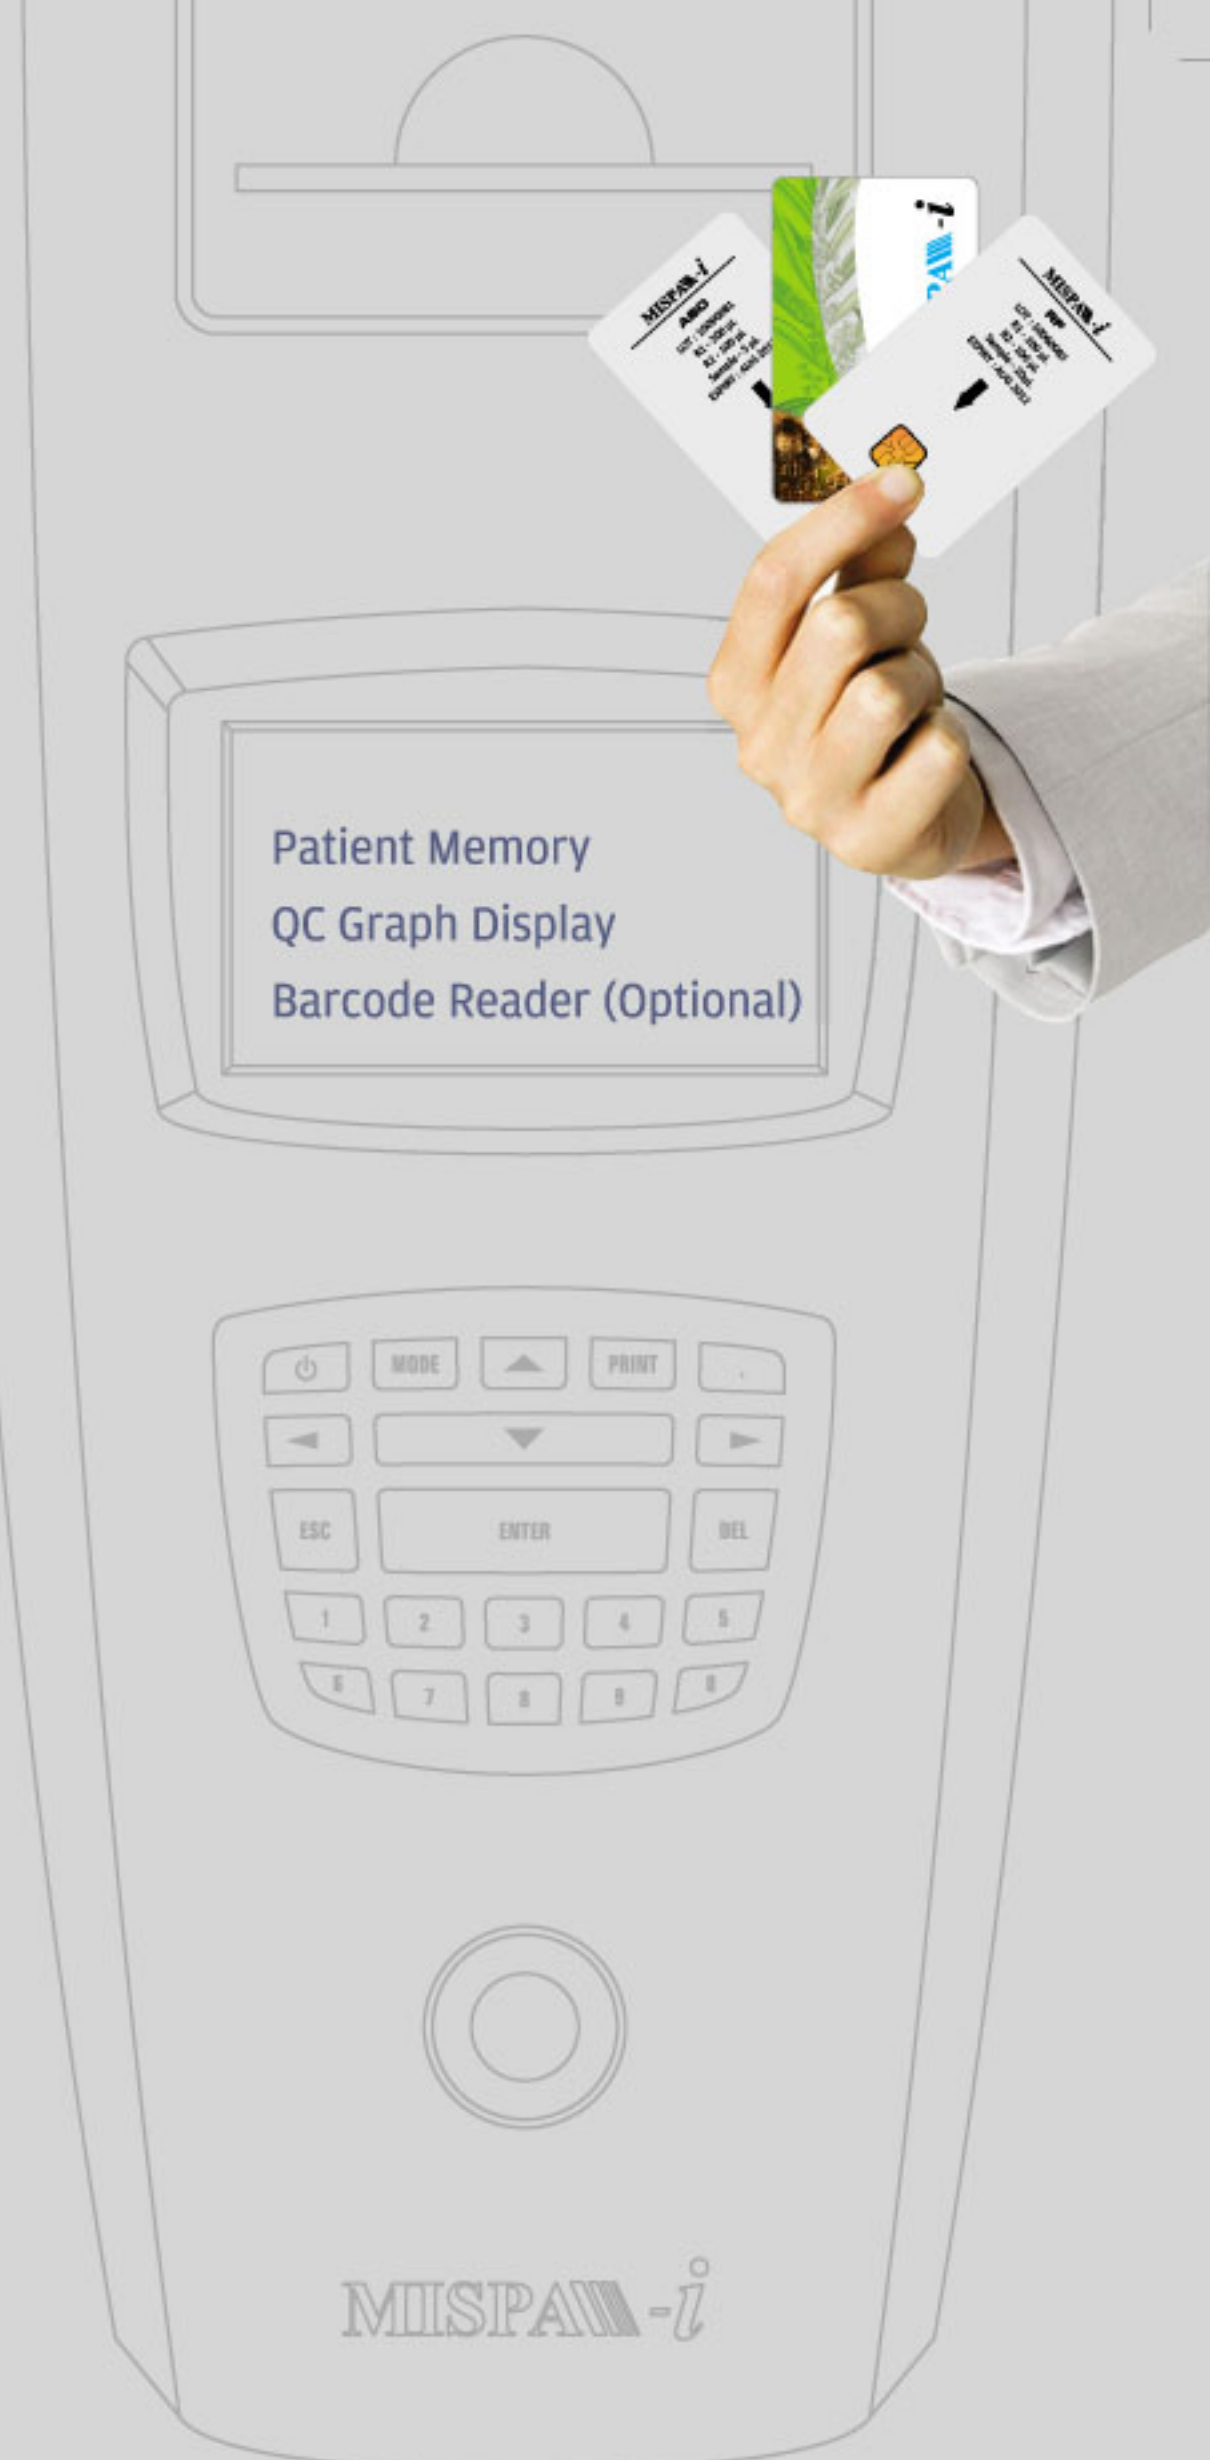

AGAPPE DIAGNOSTICS SWITZERLAND GmbH

Knounerstrasse 54 - 6330 Cham - Switzerland. Tel: +41 41 780 60 10 Fax: +41 41 780 60 11
www.agappeswiss.com | info@agappeswiss.com